

MODEL: SP-35401 **DESCRIPTION:** 3.5 mm STEREO PLUG

FEATURES

- 4 conductor
- modular strain relief




SPECIFICATIONS

| parameter | conditions/description | min | typ | max | units |
|-----------------------|-------------------------|-----|-----|-----|-------|
| contact resistance | | | | 30 | mΩ |
| insulation resistance | at 500 Vdc | 100 | | | MΩ |
| voltage withstand | at 50/60Hz for 1 minute | | | 500 | Vac |
| operating temperature | | -25 | | 70 | °C |
| RoHS | 2011/65/EU | | | | |

MECHANICAL DRAWING

units: mm[inches]
 tolerance: ±0.3mm
 unless otherwise specified

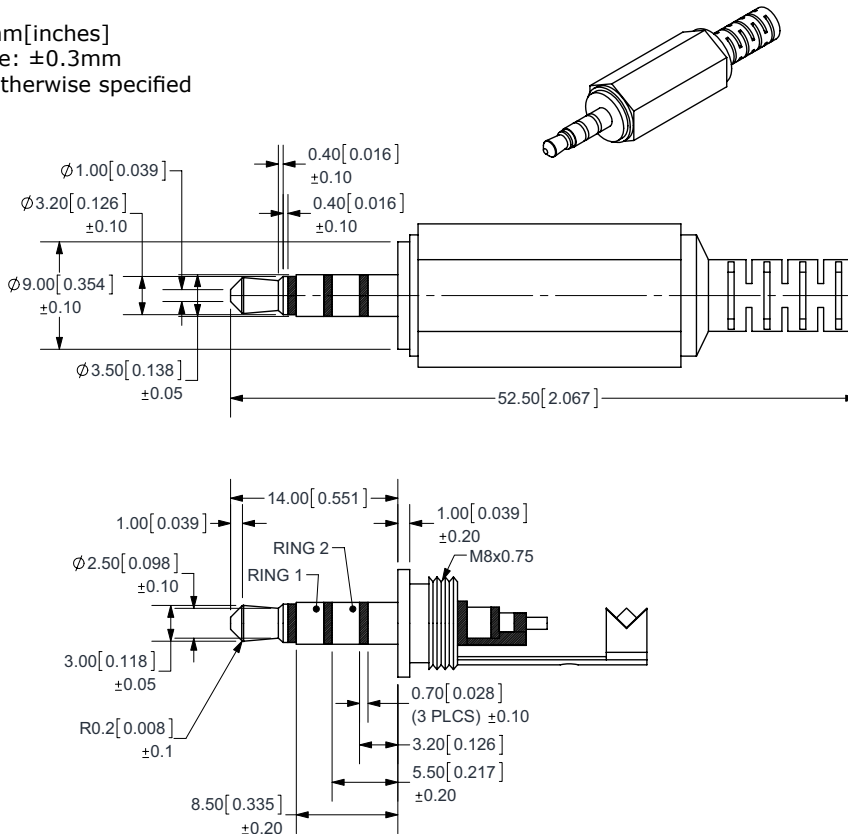

| | MATERIAL | PLATING |
|----------------|------------|-------------|
| tip | brass | nickel |
| insulator | ABS | black color |
| ring (1) | brass | nickel |
| ring (2) | brass | nickel |
| sleeve | brass | nickel |
| earth terminal | brass | nickel |
| body | PVC or TPR | black color |

Note: 1. All specifications measured at 10~35°C with a relative humidity of 45~85% under standard atmospheric pressure unless otherwise specified.

REVISION HISTORY

| rev. | description | date |
|------|------------------------------|------------|
| 1.0 | initial release | 05/05/2011 |
| 1.01 | body material changed to TPR | 08/30/2013 |

The revision history provided is for informational purposes only and is believed to be accurate.



Headquarters
20050 SW 112th Ave.
Tualatin, OR 97062
800.275.4899

Fax 503.612.2383
cui.com
techsupport@cui.com

CUI offers a one (1) year limited warranty. Complete warranty information is listed on our website.

CUI reserves the right to make changes to the product at any time without notice. Information provided by CUI is believed to be accurate and reliable. However, no responsibility is assumed by CUI for its use, nor for any infringements of patents or other rights of third parties which may result from its use.

CUI products are not authorized or warranted for use as critical components in equipment that requires an extremely high level of reliability. A critical component is any component of a life support device or system whose failure to perform can be reasonably expected to cause the failure of the life support device or system, or to affect its safety or effectiveness.